

1000 μm

FIG. 1

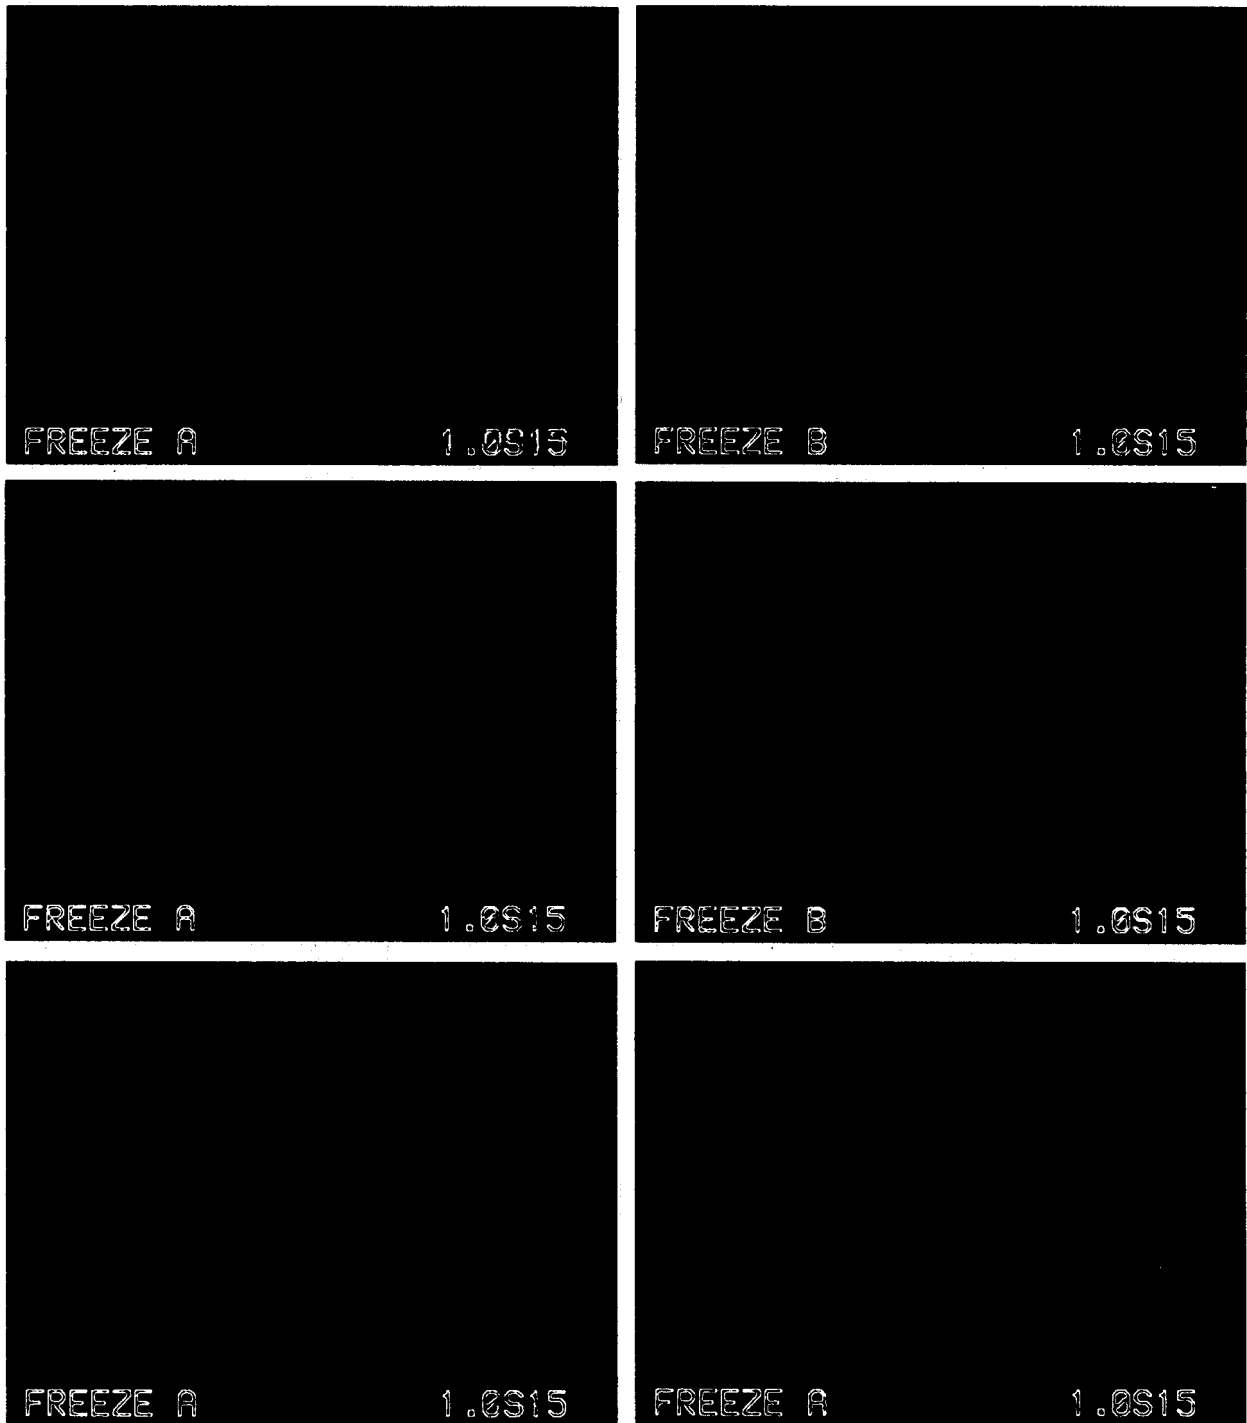


FIG. 2

+ DAPI



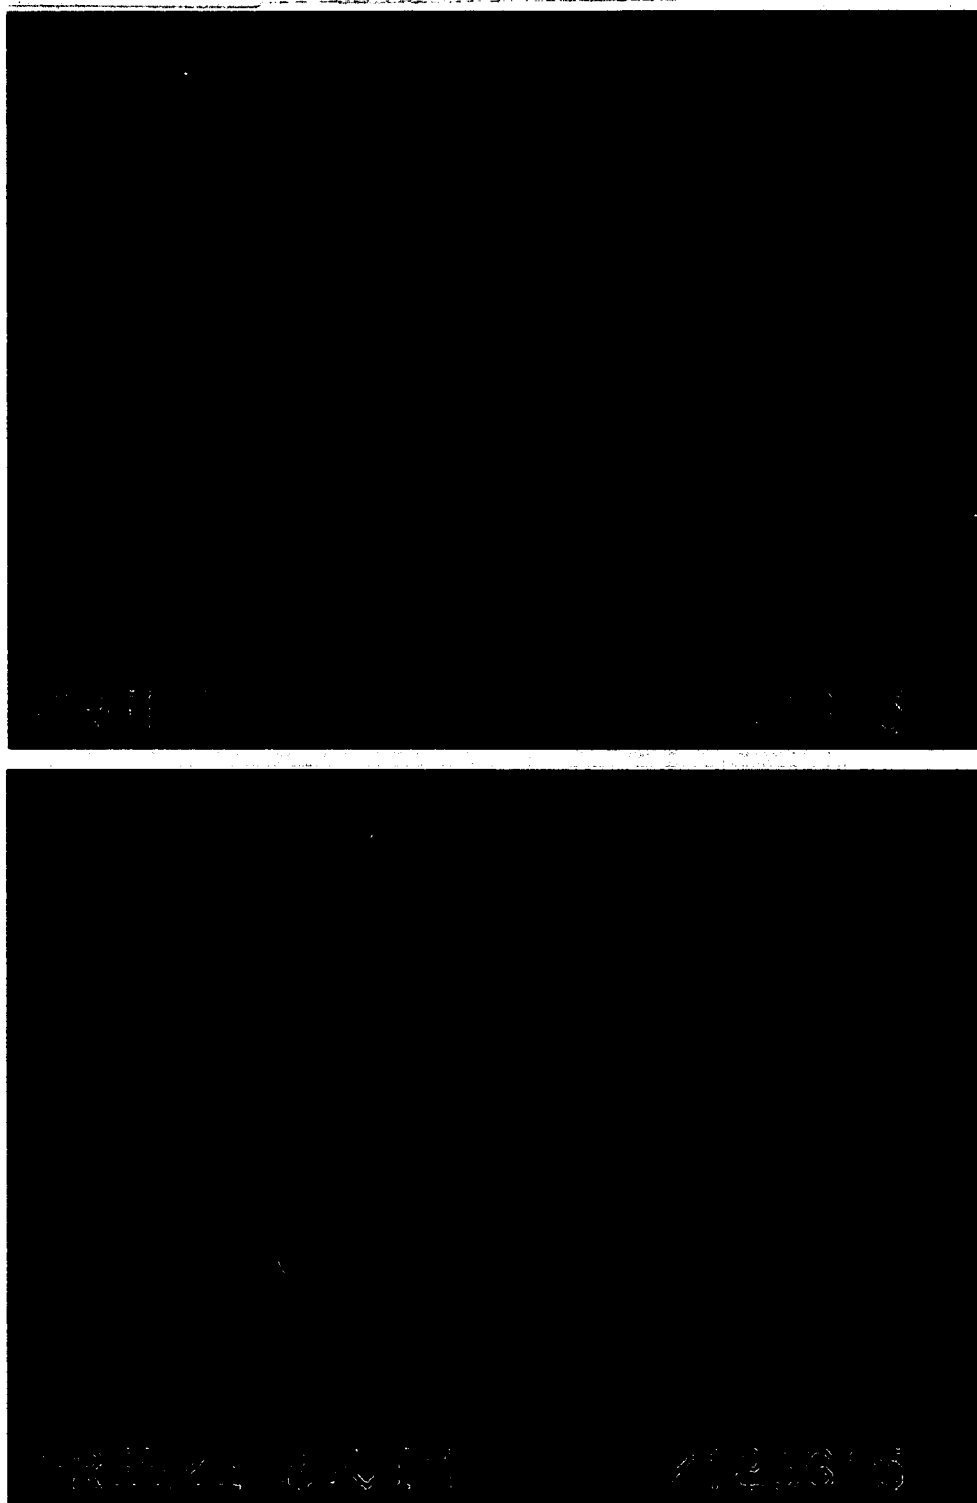


FIG. 3

Transduction

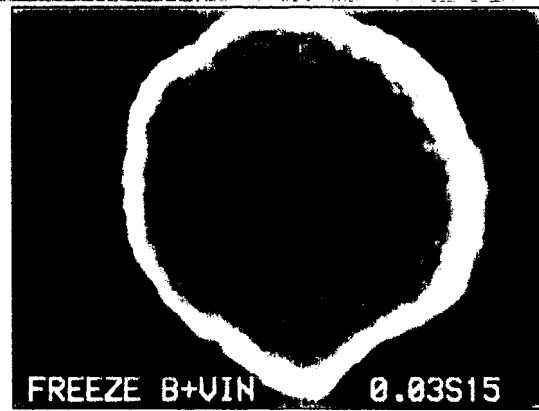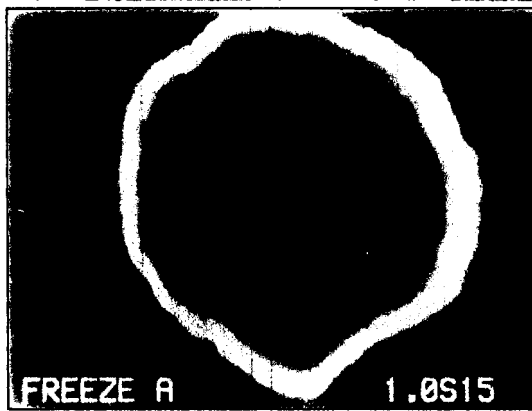

Chemicon



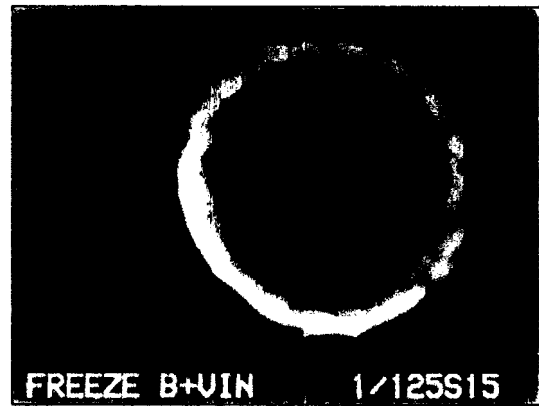


FIG. 5

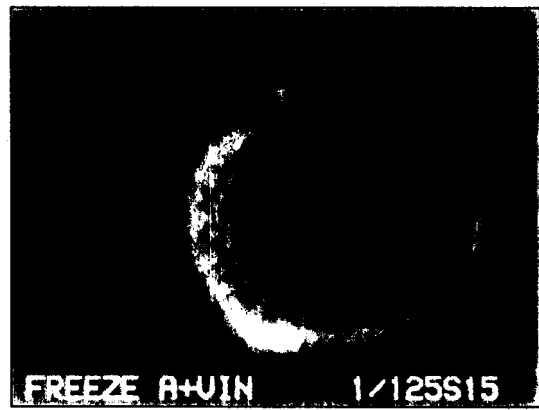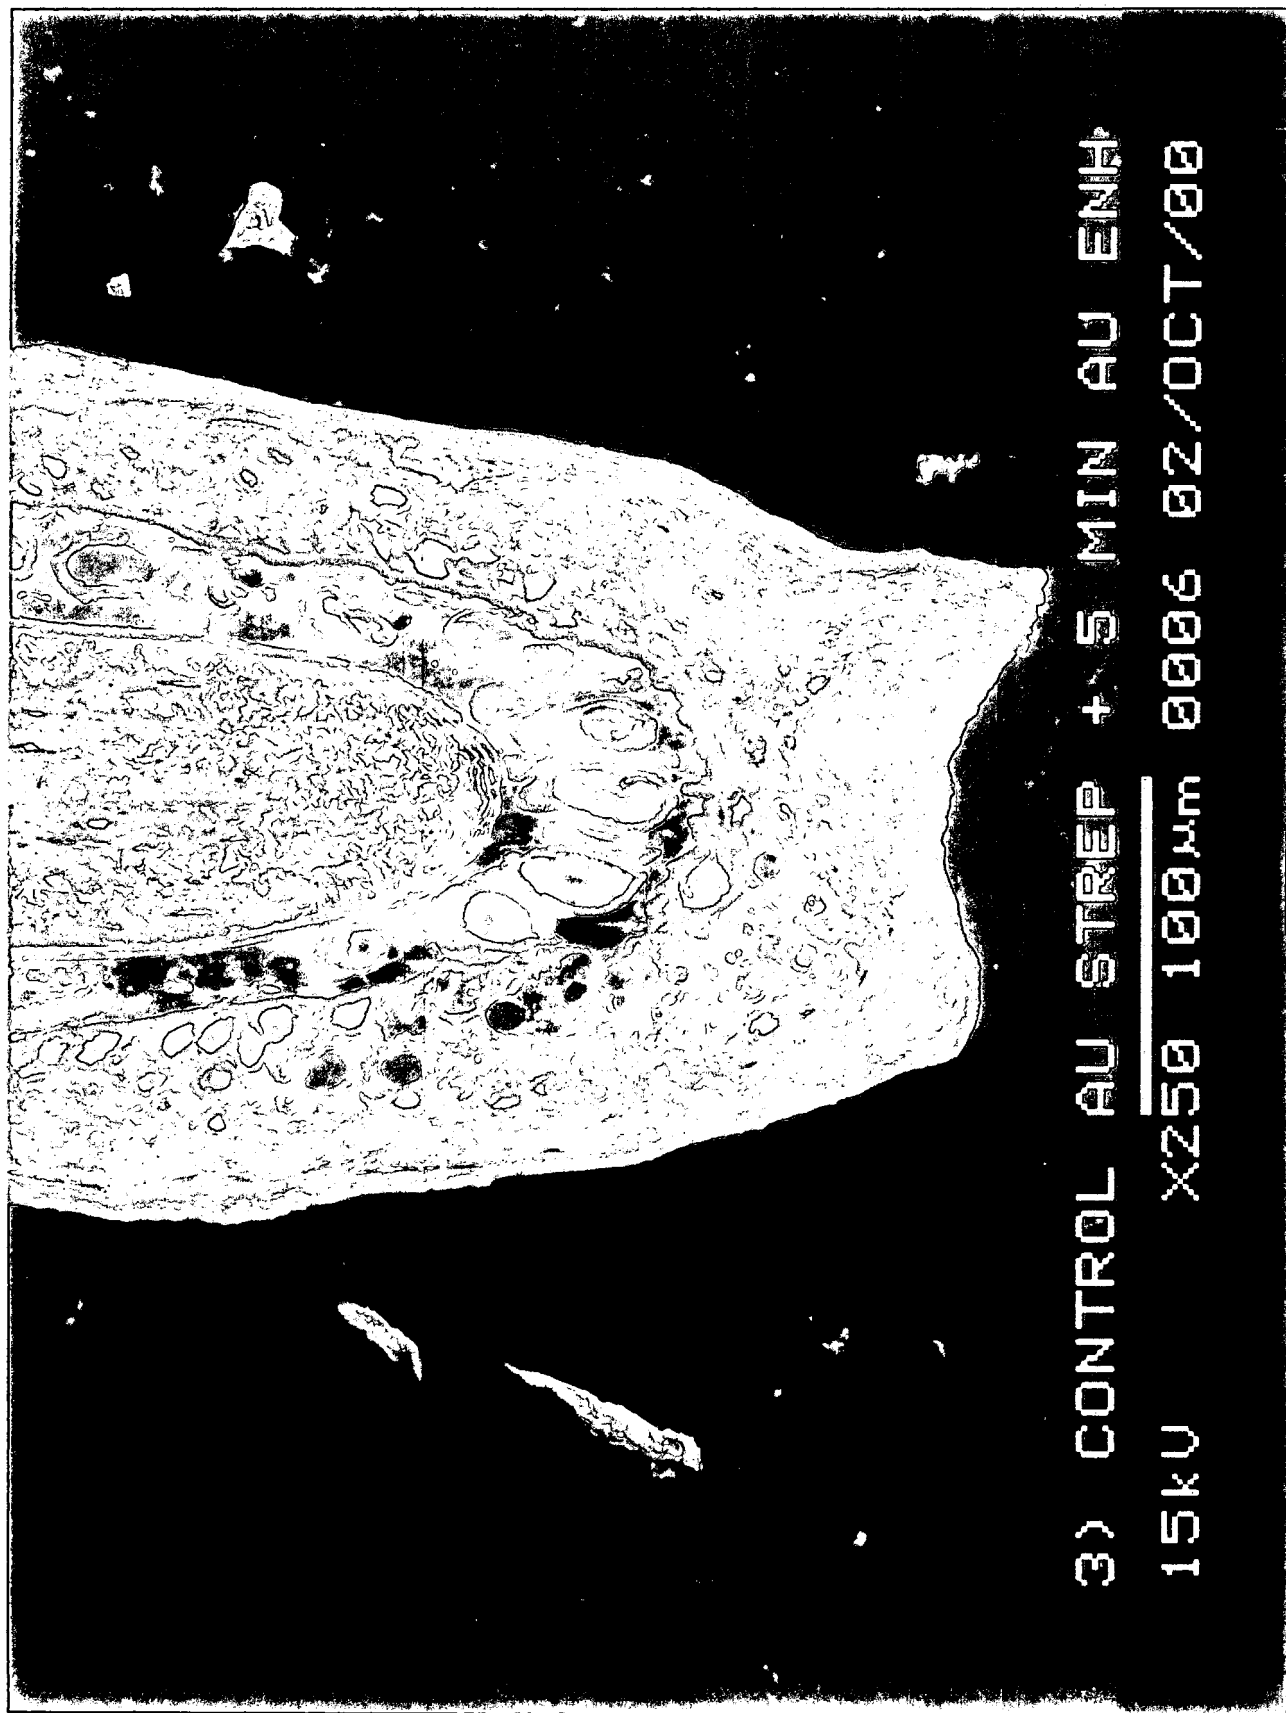

3) CONTROL AU STREP + 5 MIN AU ENH
15kV X250 100um 0006 02/OCT/00

FIG. 6

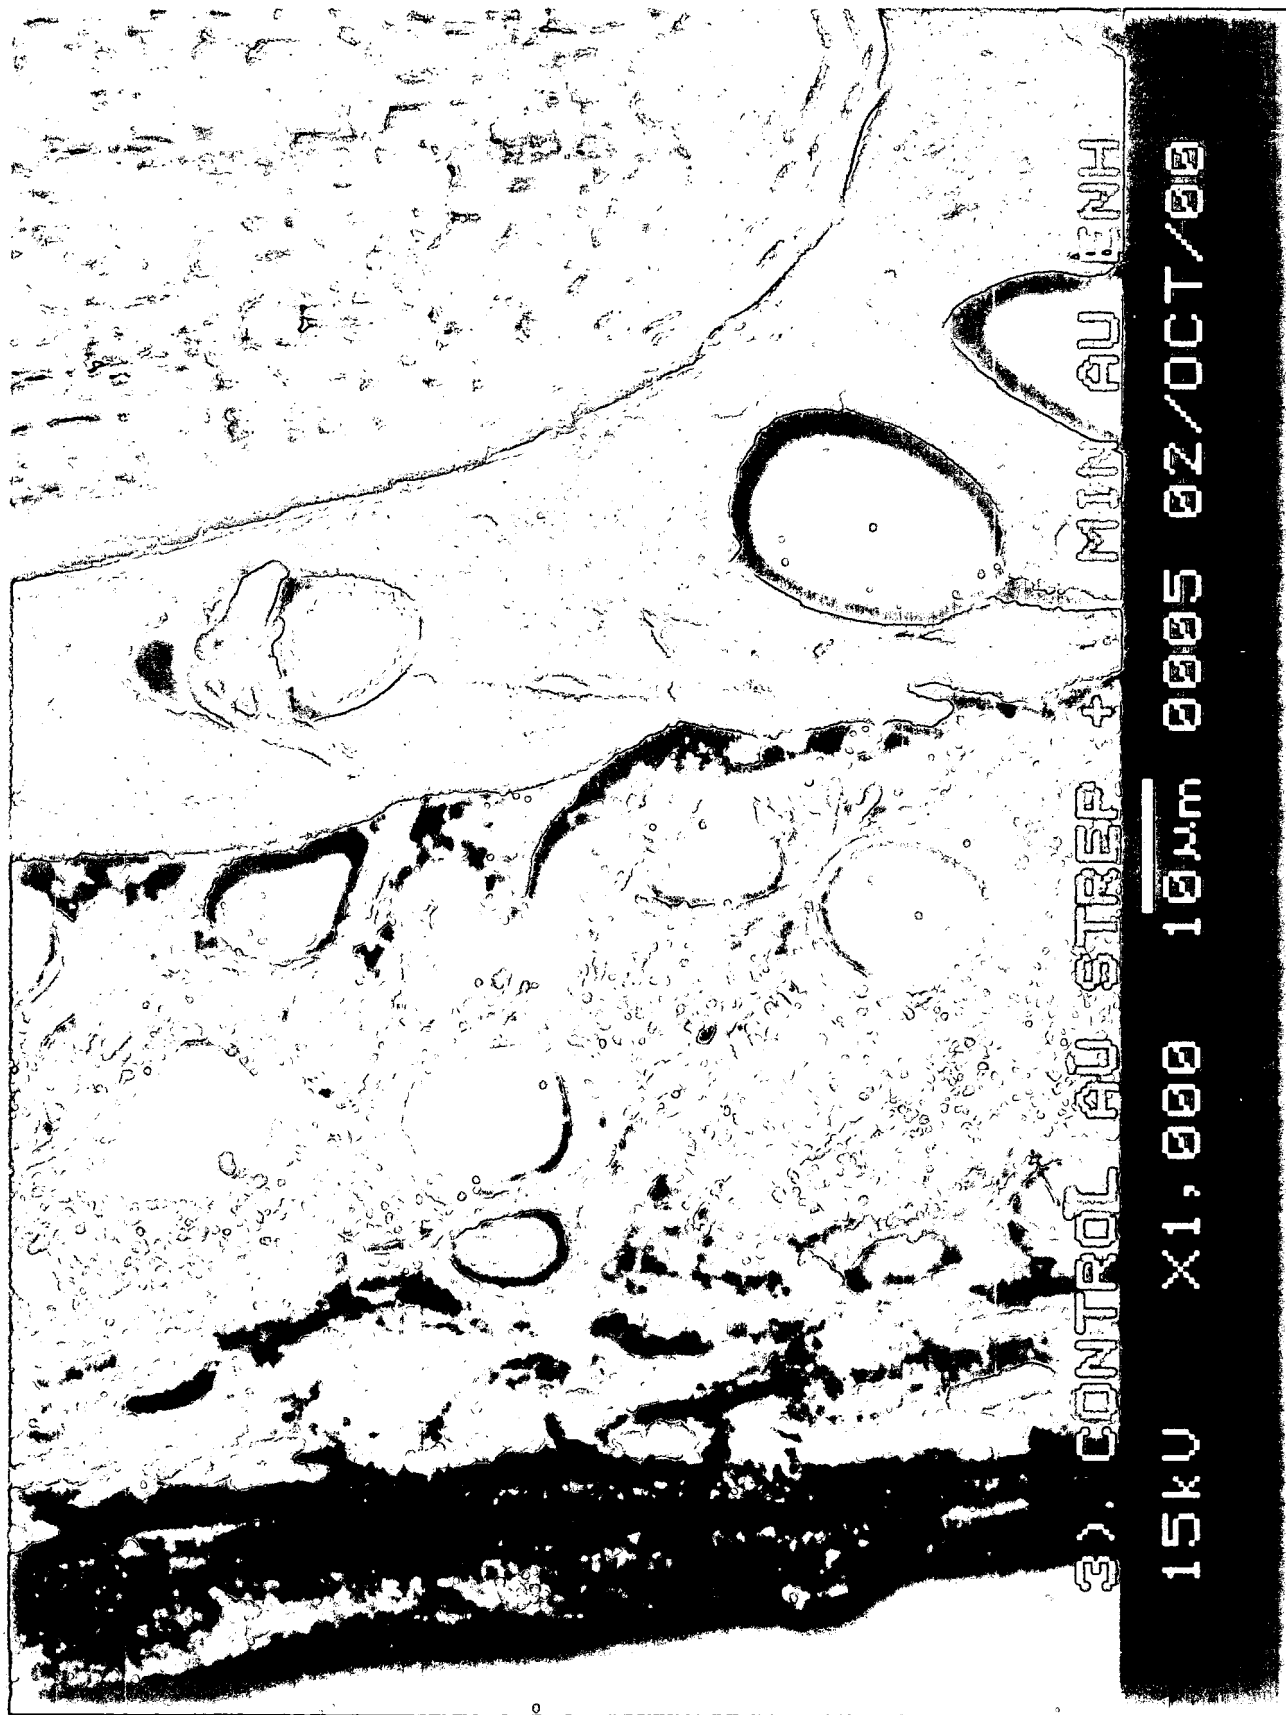


FIG. 7

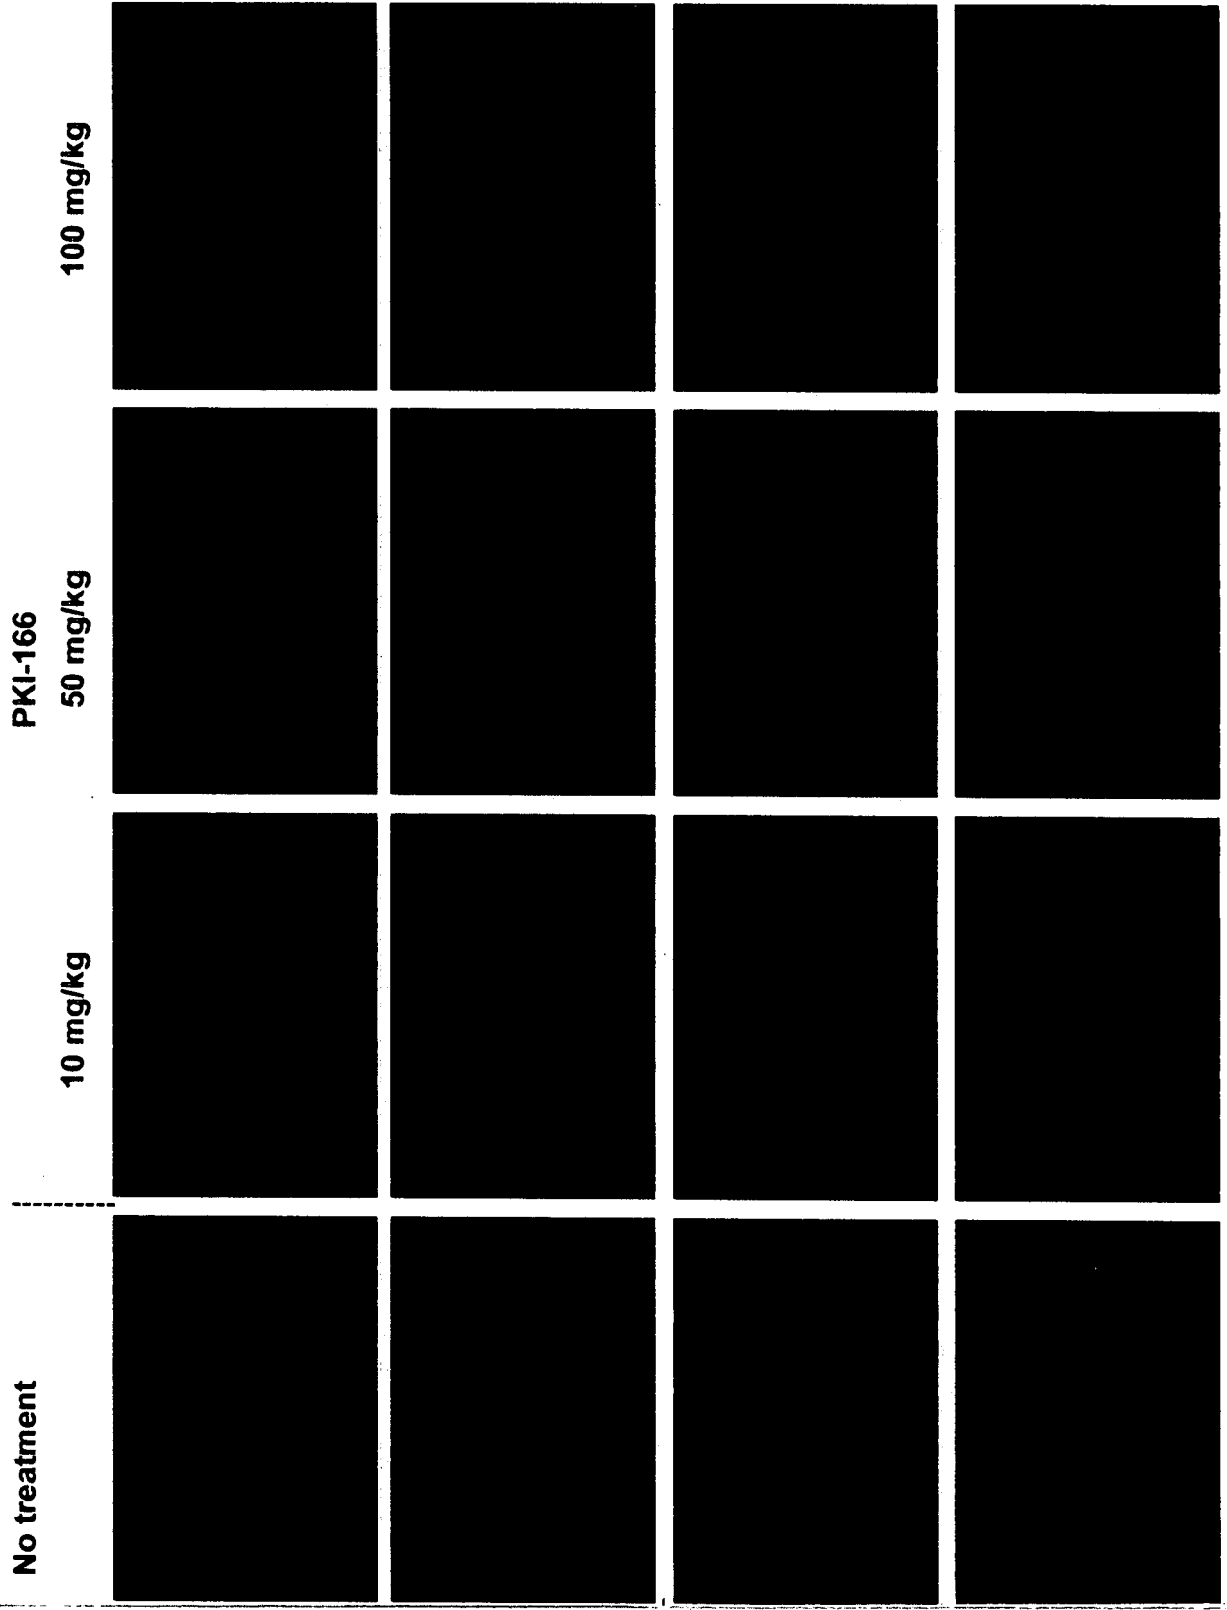


FIG. 8